

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0092
Location:	VERONA POLICE DEPT.	
Calibration File No.:	00429	Calib. Date: 12/20/2016
Certification File No.:	00430	Calib. No.: 00029
Linearity File No.:	00431	Cert. Date: 12/20/2016
Solution File No.:	00434	Cert. No.: 00020
Sequential File No.:	00434	Lin. Date: 12/20/2016
		Lin. No.: 00020
		Soln. Date: 01/25/2017
		Soln. No.: 00141
		File Date: 01/25/2017
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0065
Solution Control Lot:	16150	Expires: 07/06/2018
		Bottle No.: 0276

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:16S		
Control 1 EC	0.098%	03:16S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	03:16S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:17S		
Control 2 EC	0.097%	03:18S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	03:18S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:18S		
Control 3 EC	0.097%	03:19S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	03:19S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:20S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CARATTINI JR.

First Name: HERIBERTO

MI: -

Signature: _____

Badge No.: 9942

Date: 01/25/2017

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0092
Location:	VERONA POLICE DEPT.	
Calibration File No.:	00429	Calib. Date: 12/20/2016
Certification File No.:	00430	Calib. No.: 00029
Linearity File No.:	00431	Cert. Date: 12/20/2016
Solution File No.:	00437	Cert. No.: 00020
Sequential File No.:	00437	Lin. Date: 12/20/2016
		Lin. No.: 00020
		Soln. Date: 02/23/2017
		Soln. No.: 00142
		File Date: 02/23/2017
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0065
Solution Control Lot:	16150	Expires: 07/06/2018
		Bottle No.: 0330

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:42S		
Control 1 EC	0.100%	03:42S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	03:42S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:43S		
Control 2 EC	0.098%	03:44S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	03:44S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:45S		
Control 3 EC	0.097%	03:45S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	03:45S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:46S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CARATTINI JR.

First Name: HERIBERTO

MI: -

Signature: _____

Badge No.: 9942

Date: 02/23/2017

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: VERONA POLICE DEPT. Serial No.: ARWM-0092
Calibration File No.: 00429 Calib. Date: 12/20/2016 Calib. No.: 00029
Certification File No.: 00430 Cert. Date: 12/20/2016 Cert. No.: 00020
Linearity File No.: 00431 Lin. Date: 12/20/2016 Lin. No.: 00020
Solution File No.: 00445 Soln. Date: 03/25/2017 Soln. No.: 00143
Sequential File No.: 00445 File Date: 03/25/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXA S3-0065
Control Solution %: 0.100% Expires: 07/06/2018
Solution Control Lot: 16150 Bottle No.: 0267

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:32S		
Control 1 EC	0.097%	01:32S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	01:32S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:33S		
Control 2 EC	0.097%	01:34S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	01:34S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:35S		
Control 3 EC	0.098%	01:35S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	01:35S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:36S		

All tests within acceptable tolerance.

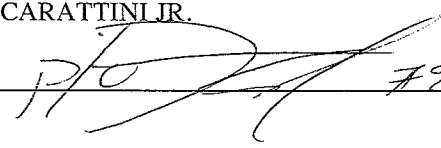
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CARATTINI JR.

First Name: HERIBERTO

MI: -

Signature: 

Badge No.: 9942

Date: 03/25/2017

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0092
Location:	VERONA POLICE DEPT.	
Calibration File No.:	00429	Calib. Date: 12/20/2016
Certification File No.:	00430	Calib. No.: 00029
Linearity File No.:	00431	Cert. Date: 12/20/2016
Solution File No.:	00453	Cert. No.: 00020
Sequential File No.:	00453	Lin. Date: 12/20/2016
		Lin. No.: 00020
		Soln. Date: 04/23/2017
		Soln. No.: 00144
		File Date: 04/23/2017
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0065
Solution Control Lot:	16150	Expires: 07/06/2018
		Bottle No.: 0765

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:46D		
Control 1 EC	0.100%	04:46D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	04:46D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:47D		
Control 2 EC	0.099%	04:47D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	04:47D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:48D		
Control 3 EC	0.099%	04:49D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	04:49D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:49D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CARATTINI JR.

First Name: HERIBERTO

MI: -

Signature: _____

Badge No.: 9942

Date: 04/23/2017

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0092
Location:	VERONA POLICE DEPT.	
Calibration File No.:	00460	Calib. Date: 05/23/2017
Certification File No.:	00461	Calib. No.: 00030
Linearity File No.:	00462	Cert. Date: 05/23/2017
Solution File No.:	00468	Cert. No.: 00021
Sequential File No.:	00468	Lin. Date: 05/23/2017
		Lin. No.: 00021
		Soln. Date: 06/23/2017
		Soln. No.: 00146
		File Date: 06/23/2017
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0068
Solution Control Lot:	16150	Expires: 07/06/2018
		Bottle No.: 0303

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:18D		
Control 1 EC	0.098%	02:18D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	02:18D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:19D		
Control 2 EC	0.098%	02:20D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	02:20D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:20D		
Control 3 EC	0.097%	02:21D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	02:21D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:22D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CARATTINI JR.

First Name: HERIBERTO

MI: -

Signature: _____

Badge No.: 9942

Date: 06/23/2017

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWM-0092
Location: VERONA POLICE DEPT.
Calibration File No.: 00460 Calib. Date: 05/23/2017 Calib. No.: 00030
Certification File No.: 00461 Cert. Date: 05/23/2017 Cert. No.: 00021
Linearity File No.: 00462 Lin. Date: 05/23/2017 Lin. No.: 00021
Solution File No.: 00477 Soln. Date: 07/23/2017 Soln. No.: 00147
Sequential File No.: 00477 File Date: 07/23/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXA S3-0068
Control Solution %: 0.100% Expires: 01/30/2019
Solution Control Lot: 17050 Bottle No.: 0096

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:11D		
Control 1 EC	0.098%	02:12D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	02:12D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:12D		
Control 2 EC	0.098%	02:13D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	02:13D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:14D		
Control 3 EC	0.098%	02:14D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	02:14D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:15D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CARATTINI JR.

First Name: HERIBERTO

MI: -

Signature: 

Badge No.: 9942

Date: 07/23/2017

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWM-0092
Location: VERONA POLICE DEPT.
Calibration File No.: 00460 Calib. Date: 05/23/2017 Calib. No.: 00030
Certification File No.: 00461 Cert. Date: 05/23/2017 Cert. No.: 00021
Linearity File No.: 00462 Lin. Date: 05/23/2017 Lin. No.: 00021
Solution File No.: 00481 Soln. Date: 09/19/2017 Soln. No.: 00149
Sequential File No.: 00481 File Date: 09/19/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXA S3-0068
Control Solution %: 0.100% Expires: 01/30/2019
Solution Control Lot: 17050 Bottle No.: 0120

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:47D		
Control 1 EC	0.100%	13:48D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:48D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:49D		
Control 2 EC	0.099%	13:49D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:50D		
Control 3 EC	0.099%	13:51D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:51D		

All tests within acceptable tolerance.

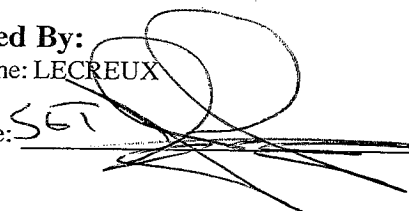
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LECREUX

First Name: JOHN

MI: C

Signature: 

Badge No.: 8776

Date: 09/19/2017

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWM-0092
Location:	VERONA POLICE DEPT.		
Calibration File No.:	00460	Calib. Date:	05/23/2017
Certification File No.:	00461	Cert. Date:	05/23/2017
Linearity File No.:	00462	Lin. Date:	05/23/2017
Solution File No.:	00489	Soln. Date:	10/21/2017
Sequential File No.:	00489	File Date:	10/21/2017

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDXA S3-0068
Control Solution %:	0.100%			Expires:	01/30/2019
Solution Control Lot:	17050			Bottle No.:	0089

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:42D		
Control 1 EC	0.099%	03:42D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	03:42D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:43D		
Control 2 EC	0.098%	03:43D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	03:43D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:44D		
Control 3 EC	0.098%	03:45D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	03:45D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:45D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

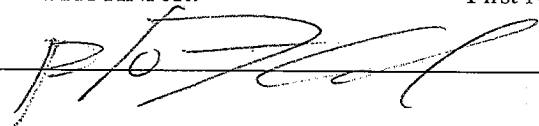
Changed By:

Last Name: CARATTINI JR.

First Name: HERIBERTO

MI: -

Signature: _____



Badge No.: 9942

Date: 10/21/2017

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWM-0092
Location: VERONA POLICE DEPT.
Calibration File No.: 00490 Calib. Date: 10/24/2017 Calib. No.: 00031
Certification File No.: 00491 Cert. Date: 10/24/2017 Cert. No.: 00022
Linearity File No.: 00492 Lin. Date: 10/24/2017 Lin. No.: 00022
Solution File No.: 00499 Soln. Date: 11/20/2017 Soln. No.: 00152
Sequential File No.: 00499 File Date: 11/20/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXA S3-0065
Control Solution %: 0.100% Expires: 01/30/2019
Solution Control Lot: 17050 Bottle No.: 0081

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:24S		
Control 1 EC	0.098%	04:25S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	04:25S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:26S		
Control 2 EC	0.096%	04:26S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	04:26S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:27S		
Control 3 EC	0.098%	04:28S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	04:28S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:28S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CARATTINI JR.

First Name: HERIBERTO

MI: -

Signature: 

Badge No.: 9942

Date: 11/20/2017

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0092
Location:	VERONA POLICE DEPT.	
Calibration File No.:	00490	Calib. Date: 10/24/2017
Certification File No.:	00491	Calib. No.: 00031
Linearity File No.:	00492	Cert. Date: 10/24/2017
Solution File No.:	00506	Cert. No.: 00022
Sequential File No.:	00506	Lin. Date: 10/24/2017
		Lin. No.: 00022
		Soln. Date: 12/19/2017
		Soln. No.: 00153
		File Date: 12/19/2017
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0065
Solution Control Lot:	17360	Expires: 10/17/2019
		Bottle No.: 0122

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:26S		
Control 1 EC	0.099%	03:27S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	03:27S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:27S		
Control 2 EC	0.098%	03:28S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	03:28S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:29S		
Control 3 EC	0.100%	03:29S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	03:29S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:30S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CARATTINI JR.

First Name: HERIBERTO

MI: -

Signature: _____

Badge No.: 9942

Date: 12/19/2017