

Calibrating Unit

New Standard Solution Report

| | | |
|-------------------------|-----------------------|--------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARWM-0092 |
| Location: | VERONA POLICE DEPT. | |
| Calibration File No.: | 00763 | Calib. Date: 12/08/2022 |
| Certification File No.: | 00764 | Cert. No.: 00046 |
| Linearity File No.: | 00765 | Cert. Date: 12/08/2022 |
| Solution File No.: | 00785 | Lin. No.: 00036 |
| Sequential File No.: | 00785 | Lin. Date: 12/08/2022 |
| | | Soln. No.: 00231 |
| | | Soln. Date: 04/01/2023 |
| | | File Date: 04/01/2023 |
| | | |
| Calibrating Unit: | WET | Model No.: CU-34 |
| Control Solution %: | 0.100% | Serial No.: DDXA S3-0065 |
| Solution Control Lot: | 22160 | Expires: 05/09/2024 |
| | | Bottle No.: 0226 |

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 23:41S | | |
| Control 1 EC | 0.101% | 23:41S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.100% | 23:41S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 23:42S | | |
| Control 2 EC | 0.100% | 23:43S | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.100% | 23:43S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 23:43S | | |
| Control 3 EC | 0.100% | 23:44S | 33.9°C | *** TEST PASSED *** |
| Control 3 IR | 0.099% | 23:44S | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 23:45S | | |

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CARATTINI JR.

First Name: H.

MI: -

Signature:  #9942

Badge No.: 9942

Date: 04/01/2023

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWM-0092
Location: VERONA POLICE DEPT.
Calibration File No.: 00786 Calib. Date: 04/06/2023 Calib. No.: 00047
Certification File No.: 00787 Cert. Date: 04/06/2023 Cert. No.: 00037
Linearity File No.: 00788 Lin. Date: 04/06/2023 Lin. No.: 00037
Solution File No.: 00794 Soln. Date: 05/04/2023 Soln. No.: 00233
Sequential File No.: 00794 File Date: 05/04/2023

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXA S3-0068
Control Solution %: 0.100% Expires: 05/09/2024
Solution Control Lot: 22160 Bottle No.: 0326

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 01:04D | | |
| Control 1 EC | 0.101% | 01:05D | 33.9°C | *** TEST PASSED *** |
| Control 1 IR | 0.100% | 01:05D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 01:06D | | |
| Control 2 EC | 0.100% | 01:06D | 33.9°C | *** TEST PASSED *** |
| Control 2 IR | 0.100% | 01:06D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 01:07D | | |
| Control 3 EC | 0.099% | 01:08D | 33.9°C | *** TEST PASSED *** |
| Control 3 IR | 0.100% | 01:08D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 01:08D | | |

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CARATTINI JR.

First Name: H.

MI: -

Signature: 

Badge No.: 9942

Date: 05/04/2023

Calibrating Unit

New Standard Solution Report

| | | |
|-------------------------|-----------------------|-------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARWM-0092 |
| Location: | VERONA POLICE DEPT. | |
| Calibration File No.: | 00786 | Calib. Date: 04/06/2023 |
| Certification File No.: | 00787 | Calib. No.: 00047 |
| Linearity File No.: | 00788 | Cert. Date: 04/06/2023 |
| Solution File No.: | 00798 | Cert. No.: 00037 |
| Sequential File No.: | 00798 | Lin. Date: 04/06/2023 |
| | | Lin. No.: 00037 |
| | | Soln. Date: 06/02/2023 |
| | | Soln. No.: 00235 |
| | | File Date: 06/02/2023 |

| | | |
|-----------------------------|------------------|--------------------------|
| Calibrating Unit: WET | Model No.: CU-34 | Serial No.: DDXA S3-0068 |
| Control Solution %: 0.100% | | Expires: 05/09/2024 |
| Solution Control Lot: 22160 | | Bottle No.: 0107 |

| Function | Result %BAC | Time HH:MM | Temperature Simulator (°C) | Comment(s) or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000% | 03:15D | | |
| Control 1 EC | 0.101% | 03:15D | 33.9°C | *** TEST PASSED *** |
| Control 1 IR | 0.101% | 03:15D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 03:16D | | |
| Control 2 EC | 0.101% | 03:16D | 33.9°C | *** TEST PASSED *** |
| Control 2 IR | 0.100% | 03:16D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 03:17D | | |
| Control 3 EC | 0.101% | 03:18D | 33.9°C | *** TEST PASSED *** |
| Control 3 IR | 0.100% | 03:18D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 03:19D | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CARATTINI JR.

First Name: H.


MI: -

Signature: _____

[Handwritten Signature] #9942

Badge No.: 9942

Date: 06/02/2023



Calibrating Unit New Standard Solution Report

| | | |
|-------------------------|-----------------------|--------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARWM-0092 |
| Location: | VERONA POLICE DEPT. | |
| Calibration File No.: | 00786 | Calib. Date: 04/06/2023 |
| Certification File No.: | 00787 | Calib. No.: 00047 |
| Linearity File No.: | 00788 | Cert. Date: 04/06/2023 |
| Solution File No.: | 00802 | Cert. No.: 00037 |
| Sequential File No.: | 00802 | Lin. Date: 04/06/2023 |
| | | Lin. No.: 00037 |
| | | Soln. Date: 07/03/2023 |
| | | Soln. No.: 00236 |
| | | File Date: 07/03/2023 |
| | | |
| Calibrating Unit: | WET | Model No.: CU-34 |
| Control Solution %: | 0.100% | Serial No.: DDXA S3-0068 |
| Solution Control Lot: | 22160 | Expires: 05/09/2024 |
| | | Bottle No.: 0164 |

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 01:21D | | |
| Control 1 EC | 0.100% | 01:22D | 33.9°C | *** TEST PASSED *** |
| Control 1 IR | 0.100% | 01:22D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 01:22D | | |
| Control 2 EC | 0.099% | 01:23D | 33.9°C | *** TEST PASSED *** |
| Control 2 IR | 0.100% | 01:23D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 01:24D | | |
| Control 3 EC | 0.100% | 01:24D | 33.9°C | *** TEST PASSED *** |
| Control 3 IR | 0.099% | 01:24D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 01:25D | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CARATTINI JR.

First Name: H.

MI: -

Signature: _____

Badge No.: 9942

Date: 07/03/2023

Calibrating Unit

New Standard Solution Report

| | | |
|-------------------------|-----------------------|--------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARWM-0092 |
| Location: | VERONA POLICE DEPT. | |
| Calibration File No.: | 00786 | Calib. Date: 04/06/2023 |
| Certification File No.: | 00787 | Calib. No.: 00047 |
| Linearity File No.: | 00788 | Cert. Date: 04/06/2023 |
| Solution File No.: | 00804 | Cert. No.: 00037 |
| Sequential File No.: | 00804 | Lin. Date: 04/06/2023 |
| | | Lin. No.: 00037 |
| | | Soln. Date: 08/02/2023 |
| | | Soln. No.: 00237 |
| | | File Date: 08/02/2023 |
| | | |
| Calibrating Unit: | WET | Model No.: CU-34 |
| Control Solution %: | 0.100% | Serial No.: DDXA S3-0068 |
| Solution Control Lot: | 22160 | Expires: 05/09/2024 |
| | | Bottle No.: 0118 |

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 02:36D | | |
| Control 1 EC | 0.101% | 02:37D | 33.9°C | *** TEST PASSED *** |
| Control 1 IR | 0.101% | 02:37D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 02:38D | | |
| Control 2 EC | 0.100% | 02:38D | 33.9°C | *** TEST PASSED *** |
| Control 2 IR | 0.100% | 02:38D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 02:39D | | |
| Control 3 EC | 0.100% | 02:40D | 33.9°C | *** TEST PASSED *** |
| Control 3 IR | 0.101% | 02:40D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 02:40D | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CARATTINI JR.

First Name: H.

MI: -

Signature: _____

Badge No.: 9942

Date: 08/02/2023

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWM-0092
Location: VERONA POLICE DEPT.
Calibration File No.: 00786 Calib. Date: 04/06/2023 Calib. No.: 00047
Certification File No.: 00787 Cert. Date: 04/06/2023 Cert. No.: 00037
Linearity File No.: 00788 Lin. Date: 04/06/2023 Lin. No.: 00037
Solution File No.: 00805 Soln. Date: 09/02/2023 Soln. No.: 00238
Sequential File No.: 00805 File Date: 09/02/2023

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXA S3-0068
Control Solution %: 0.100% Expires: 05/09/2024
Solution Control Lot: 22160 Bottle No.: 1181

| Function | Result %BAC | Time HH:MM | Temperature Simulator (°C) | Comment(s) or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000% | 01:36D | | |
| Control 1 EC | 0.101% | 01:36D | 33.9°C | *** TEST PASSED *** |
| Control 1 IR | 0.101% | 01:36D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 01:37D | | |
| Control 2 EC | 0.100% | 01:37D | 33.9°C | *** TEST PASSED *** |
| Control 2 IR | 0.100% | 01:37D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 01:38D | | |
| Control 3 EC | 0.100% | 01:39D | 33.9°C | *** TEST PASSED *** |
| Control 3 IR | 0.100% | 01:39D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 01:39D | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CARATTINI JR.

First Name: H.

MI: -

Signature: _____

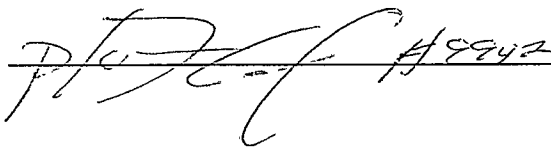

Badge No.: 9942

Date: 09/02/2023